

Signet 2724-2726 and 2734-2736 Series DryLoc pH and ORP Electrodes



3-2724.090 Rev. H 11/13

Operating Instructions

2724 & 2725 2734 & 2735 Flat Glass Electrode 2726 & 2736 Protected Bulb Glass Electrode



Description

The Signet 2724-2726 and 2734-2736 Series of pH and ORP electrodes are designed to minimize maintenance time and maximize value.

- The unique DryLoc® connector provides quick assembly and a secure connection featuring gold-plated contacts and an O-ring seal.
- The patented design features a lengthened reference chamber pathway to extend the operational life of the electrode.
- Wetted materials are selected to withstand a wide array of industrial applications.
- Multiple mounting features address the need for installation flexibility.
 These electrodes can be threaded into ¾ in. NPT or ISO 7/1 R¾ inch pipe fittings, submerged in a tank, or mounted into familiar Signet installation fittings.
- To build a stand-alone, self-contained pH control system, combine the 2724-2726 electrodes with a 2760 pH Preamplifier and add a 8750 pH/ORP Transmitter to move your control capability to the next level.
- Combine the 2427-2726 or 2734-2736 electrodes with the 2750 pH Sensor Electronics to provide a 4 to 20 mA loop to a Programmable Logic Controller (PLC), SCADA system, or datalogger.
- For more flexibility and unique features, pair the 2724-2726 or 2734-2736 series with a 2750 pH/ORP Sensor Electronics and the new 9900 Transmitter.
- Connect up to six 2724-2726 or 2734-2736 electrodes to one 8900 Multi-Parameter Controller with six 2750 pH/ORP Sensor Electronics using digital (S³L) serial data output for a truly amazing set of features, options, and measurements.
- The 2724-2726 electrodes are recommended for general purpose applications.
- The 2734-2736 electrodes are recommended for harsh applications.
- The 2734-2736 electrodes utilize advanced reference technology to extend electrode life in all applications.

Table of Contents

Description	1
Warranty Statement	2
Product Registration	2
Chemical Compatibility	2
Safety Information	2
Dimensions	3
Specifications	3
In-Line Installation	4
Low Conductivity Installation	
Signet Installation Fittings	
Removing from In-Line Installation	
Submersible Installation	
pH System Calibration	6
ORP System Calibration	6
Electrode Date Code	7
Electrode Care and Application	7
Cleaning	7
Ordering Information	8



Warranty Information

Refer to your local Georg Fischer Sales office for the most current warranty statement.

All warranty and non-warranty repairs being returned must include a fully completed Service Form and goods must be returned to your local GF Sales office or distributor. Product returned without a Service Form may not be warranty replaced or repaired.

Signet products with limited shelf-life (e.g. pH, ORP, chlorine electrodes, calibration solutions; e.g. pH buffers, turbidity standards or other solutions) are warranted out of box but not warranted against any damage, due to process or application failures (e.g. high temperature, chemical poisoning, dry-out) or mishandling (e.g. broken glass, damaged membrane, freezing and/or extreme temperatures).

Product Registration

Thank you for purchasing the Signet line of Georg Fischer measurement products.

If you would like to register your product(s), you can now register online in one of the following ways:



- Visit our website www.gfsignet.com and click on Product Registration Form

 If this is a pdf manual (digital copy) click!
 - If this is a pdf manual (digital copy), click here
 - · Scan the QR Code on the left

Chemical Compatibility

The retaining nuts of pH and ORP sensors are not designed for prolonged contact with aggressive substances. Strong acids, caustic substances and solvents or their vapor may lead to failure of the retaining nut, ejection of the sensor and loss of the process fluid with possibly serious consequences, such as damage to equipment and serious personal injury. Retaining nuts that may have been in contact with such substances, e.g. due to leakage or spilling, must be replaced.

- The use of this product assumes operators are trained and familiar with this type of device.
- Operators should be knowledgeable of the potential risks associated with pressurized piping systems.
- Operators MUST follow all necessary safety procedures.



Safety Information

- 1. Use appropriate eye, face, hand, body and/or respiratory protection when using chemicals or solvents.
- 2. Prior to installation or removal:
 - Depressurize and vent system
 - · Drain below sensor level.
- 3. Confirm chemical compatibility before use.
- 4. Do not exceed the max. temperature/pressure specifications.
- 5. Do not alter product construction.

If installing into a threaded connection:

- 6. Inspect threads to ensure integrity. Do not install a sensor that has damaged threads.
- 7. Apply PTFE tape to the process connection threads in accordance with industry practices.
- **8. HAND TIGHTEN** the sensor into the process connection. DO NOT USE TOOLS.



Caution / Warning / Danger

Indicates a potential hazard. Failure to follow all warnings may lead to equipment damage, injury, or death



Personal Protective Equipment (PPE)

Always utilize the most appropriate PPE during installation and service of Signet products.v



Pressurized System Warning

Sensor may be under pressure, take caution to vent system prior to installation or removal. Failure to do so may result in equipment damage and/or serious injury.



Hand Tighten Only

Overtightening may permanently damage product threads and lead to failure of the retaining nut.



Do Not Use Tools

Use of tool(s) may damage product beyond repair and potentially void product warranty.



Note / Technical Notes


Highlights additional information or detailed procedure.




Products are temperature sensitive and may contain freezable liquids. Freezing damage to pH. ORP. and Chlorine electrodes voids product warranty.

Dimensions


2724, 2725, 2734, & 2735 Flat Glass Electrode

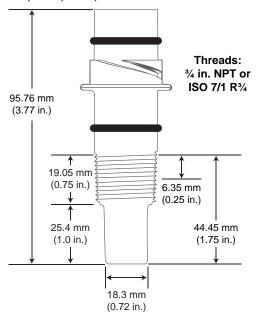

2726 & 2736 Protected Bulb Glass Electrode

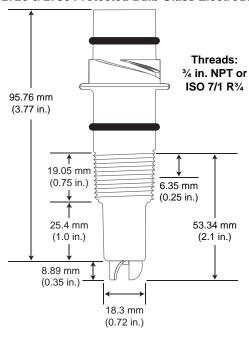

Maximum Temperature and Pressure Rating



Specifications

Ger	ne	ra
-----	----	----

•••••	
Compatibility	.2750 pH/ORP Sensor electronics,
	2760 pH/ORP preamplifier (2724-2726 only)
pH Temp Sensor:	
PT1000	. Compatible with 2750 electronics
Connection to	.PLC, 9900 Transmitter,
	8900 Multi-Parameter Controller
3 KΩ Balco	. Compatible with 2760 preamplifier
Connection to	.8750 pH/ORP Transmitter
Process Connection	.¾ in. NPT or ISO 7/1 R¾ threads
	or Signet flow fittings

Wetted Materials:

pH (2724 & 2726)Ryton (PPS), glass, UHMW PE, FPM
ORP (2725)Ryton (PPS), glass, UHMW PE, FPM,
pH (2734 & 2736)
ORP (2735)Ryton (PPS), glass, PTFE, FPM, Platinum

Shipping Weight.... 0.25 kg (0.55 lb)

Performance

Efficiency (2724-2726)....> 97% @ 25 °C (77 °F) Efficiency (2734-2736)....> 95% @ 25 °C (77 °F)

- Efficiency indicates the "wellness" of a new electrode.
- Efficiency is measured by comparing the actual slope (mV/pH) at 25 °C to the theoretical output of 59.16 mV/pH.
- An efficiency of 95% to 100% is equivalent to a slope of 56.20 to 59.16 mV/pH.

Measuring Range:

pH	0 to 14
ORP	±2000 mV
3-2726-LC	.Low Conductivity fluids (20 to 100 µS/cm)
≤ 20 µS/cm	.Flow must be less than 150 ml/min. in a properly grounded system
3-2724-HF, 3-2726-HF, 3-2734-HF, 3-2736-HF	.Hydrofluric acid resistant glass,
	pH 6 or below; trace HF ≤ 2%

For applications where hydrofluoric acid, in concentrations of 2% or less, will attack standard pH glass in levels of pH 6 and below, or in situations where process upsets may temporarily drop to these pH levels.

Environmental Requirements

Operating Temperature

2724-2726*	10 °C to 85 °C (14 °F to 185 °F)
2734-2736*	. 10 °C to 100 °C (50 °F to 212 °F)
*Best performance for 3-2724	-HF, 3-2726-HF, 3-2734-HF,

3-2736-HF is above 10 °C (50 °F)

Operating Pressure Range

2724-2726:

- 0 to 6.9 bar (0 to 100 psi) @ -10 °C to 65 °C (14 °F to 149 °F)
- Linearity Derated 6.9 to 4.0 bar (100 to 58 psi) @ 65 °C to 85 °C (149 °F to 185 °F)

2734-2736:

- 0 to 6.9 bar (0 to 100 psi) @ 10 °C to 65 °C (50 °F to 149 °F)
- Linearity Derated 6.9 to 4.0 bar (100 to 58 psi) @ 65 °C to 100 °C (149 °F to 212 °F)

Recommended storage temperature

pH/ORP electrodes......0 °C to 50 °C (32 °F to 122 °F)



- The electrode glass will shatter if shipped or stored at temperatures below 0 °C (32 °F).
 - The performance life of the electrode will be shortened if stored at temperatures above 50 °C (122 °F).

Standards and Approvals

- Manufactured under ISO 9001 for Quality, ISO 14001 for Environmental Management and OHSAS 18001 for Occupational Health and Safety.
- RoHS Compliant



China RoHS (Go to www.gfsignet.com for details)

In-Line Installation

- The electrode can be mounted at any angle.
- 2. Avoid air pockets and sediment.
- The fitting must place the electrode in the flow but must not bottom out in the pipe.
- 4. Select a Signet installation fitting for convenience.
- Use the ¾ in. threads on the electrode body to install the electrode into reducing tee fittings.
- Inspect threads to ensure integrity. Do not install an electrode with damaged threads.

Horizonta

- 7. Apply PTFE tape to the process connection threads, in accordance with industry standards.
- 8. Use piping installation hardware with smooth, well-finished threads to facilitate the installation.
- 9. If necessary, the pipe should be plumbed with a depression (trap) so liquid is maintained around the electrode tip.
- 10. Hand-tighten the electrode into the process connection. Do not use any tools to install the electrode. The use of wrenches, pliers or similar may over-stress the sensor body and lead to breakage and subsequent spillage of the process liquid.



CAUTION:


A broken sensor may be ejected forcefully from the fitting and can cause severe injury.

 The safety instructions have an adhesive label and should be placed near the sensor.




Low Conductivity Installation

- The 3-2726-LC pH electrodes can be used in low conductivity water of less than 100 μS.
- When used in the range of 20 to 100 µS, the flow range must not exceed 1 m/s (3 ft/s) velocity.
- When used in liquids of less than 20 µS, the flow range must not exceed 150 ml/min; the sensor should also be mounted in a well grounded cell.

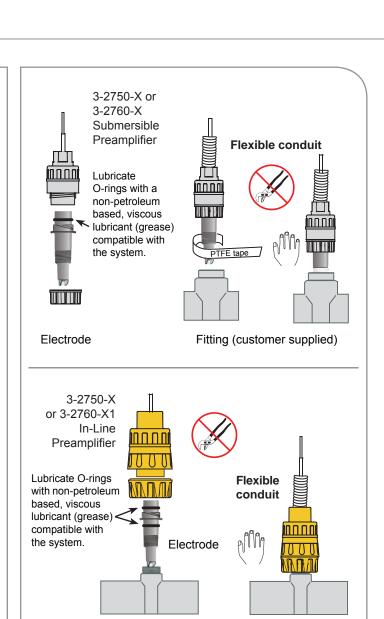


Signet Installation Fitting DN15 to DN100 (½ in. to 4 in.)

Do not use as a handle!

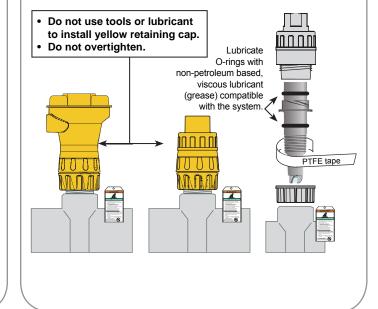

Signet Installation Fittings



Туре	Description
Carbon steel weldolets	Available in 2 in. to 4 in. sizes Requires 1-7/16 in. hole in pipe Install by certified welder only
Carbon steel threaded tees	Available in ½ in. to 2 in. sizes Female NPT ends
Universal pipe adapters	Use for installation in pipes >4 in. (1½ in. NPT) PVC, CPVC, or PVDF versions Specify socket or 1½ inch NPT male threads

Removing from In-Line Installations



- The use of this product assumes that operators are trained and are familiar with this type of device.
- They should be knowledgeable of the potential risks associated with pressurized piping systems.
- Operators MUST follow all necessary safety procedures.

In-line removal Instructions:


- 1. Depressurize and vent the piping system.
- 2. Drain the system to below sensor level.
- Wear safety goggles or face shield during removal.
 Use all appropriate eye, face, hand, body and/or respiratory protection when working with chemicals or solvents.
- 4. Place a Lockout tag on the pipe when the sensor is removed for maintenance to prevent accidental opening and exposure to potentially hazardous chemicals.

Submersible Installations

The user must supply the following hardware to complete a submersible installation:


- ¾ in. NPT threaded pipe or conduit
- Wiring junction box
- · Pipe clamps (quick-release type recommended)
- Tank flange for closed tanks


Technical Note:




- Use the ¾ in. threads at the top of the preamplifier to run the cable inside pipe or conduit.
- Place the electrode tip in pH 4 buffer during system maintenance or storage to avoid dehydration.

2724-2726 / 2734-2736 with 2750/2760 Preamplifier







The Signet pH/ORP electrodes are designed to install in tanks by attaching conduit to the ¾ in. threads at the top of the accompanying preamplifier or sensor electronics:

- 1. The O-ring at the top of the electrode fits very tightly into the preamplifier. Use a small amount of non-petroleum based lubricant to assist the assembly.
- 2. To prevent moisture from migrating into the preamplifier, backfill the conduit with 3 in. to 4 in. of sealant.
- 3. Mount electrodes in a location with ample clearance to remove them for periodic cleaning and recalibration.
- 4. Choose a location that keeps the electrode glass completely submersed at all times.

pH System Calibration

There are two functions in a pH electrode that require the system to be calibrated:

Temperature

- The temperature output of the electrode (from a 3K Balco or PT1000 RTD) must be calibrated only once.
 When a new electrode is installed, it does not need to be repeated.
- Because the temperature measurement has a significant influence on the electrochemical measurement, the temperature output in new pH electrodes should always be calibrated before the pH/mV calibration.

NOTE: All Signet transmitters and controllers incorporate automatic temperature compensation.

	pH error due to temperature changes in fluid										
°C	pH 2	pH 3	pH 4	pH 5	pH 6	pH 7	pH 8	pH 9	pH 10	pH 11	pH 12
15	0.15	0.12	0.09	**0.06	0.03	0	0.03	0.06	0.09	0.12	0.15
25	0	0	0	* 0	0	0	0	0	0	0	0
35	0.15	0.12	0.09	0.06	0.03	0	0.03	0.06	0.09	0.12	0.15
45	0.3	0.24	0.18	0.12	0.06	0	0.06	0.12	0.18	0.24	0.3
55	0.45	0.36	0.27	0.18	0.09	0	0.09	0.18	0.27	0.36	0.45

Table 1

As the pH value moves away from neutral (7 pH) or the temperature moves away from 25 $^{\circ}$ C, the electrochemical output is affected.

- * Example: At pH 5 the mV output of the electrode is not affected if the temperature is at 25 °C.
- ** The electrode output will be shifted by 0.06 pH units if the temperature is reduced to 15 °C.

Electrochemical pH vs. mV Ratio

- The mV output from the electrode is created by the interaction of the electrode and the fluid.
- The electrode contains a gel that depletes over time, so the instrument must be readjusted periodically to maintain system accuracy.
- · The need for recalibration varies with each application, but the life of the electrode is usually consistent.
- Keep a maintenance log to establish a depletion trend in new systems.
- The mV calibration is a two-point procedure.
- Signet offers pH buffer solutions prepared specifically for this purpose.
- pH buffer solutions can be used for calibrating more than one sensor within a day provided that the solutions are protected from debris and are not diluted by rinse water from the calibration procedure.
- Use clean water to rinse buffer solutions from the electrode.
- · Dispose of all buffer solutions at the end of the day.
- If the pH sensor will not calibrate within acceptable limits, clean the electrode and recalibrate.
- · If the calibration results remain outside of acceptable limits, the sensor is depleted and must be replaced.
- Follow the guidelines of local waste disposal regulations when discarding buffer solutions and spent electrodes.

	Theoretical mV Values @ 25 °C				
рН	mV				
2	+295.8				
3	+236.64				
4	+177.48				
5	+118.32				
6	+59.16				
7	0				
8	-59.16				
9	-118.32				
10	-177.48				
11	-236.64				
12	-295.8				

Table 2
Electrode slope is the ratio of mV to pH units.
At 25 °C the theoretical slope is 59.16 mV per pH.

ORP System Calibration

ORP electrodes do not incorporate a temperature sensor, so the only system calibration required is the electrochemical adjustment.

Electrochemical ORP vs. mV Ratio

- · ORP measurements are relative values, and single-point adjustments are sufficient for most applications.
- Calibration should be done using ORP test solutions such as Zobell's solution, Light's solution, or in pH buffers that have been saturated with quinhydrone (Table 3). Quinhydrone is the oxidizer that is measured by the ORP electrode.
- Zobell's solution and Light's solution are not compatible with the AutoCal function in Signet pH instrumentation.
- A new ORP electrode measures the listed values ±15 mV.
- The ORP electrode is functional until the offset exceeds 50 mV.
- · An electrode whose offset measures greater than 50 mV should be cleaned or replaced if necessary.
- ORP solutions made with quinhydrone are very unstable and may not read properly after being exposed to air for a prolonged time. These solutions must be discarded after a few hours.
- Dispose of all calibration solutions in accordance with local, state and federal guidelines.
- Use clean water to rinse buffer solutions from the sensors.

3013.	Zobell's solution	Light's solution	4 pH buffer w/quinhydrone*	7 pH buffer w/quinhydrone*
ORP at 20 °C			268 mV	92 mV
ORP at 25 °C	228 mV	469 mV	263 mV	86 mV
ORP at 30 °C			258 mV	79 mV

Table 3: ORP test solutions

*Saturate 50 mL of pH 4 or pH 7 buffer with 1/8 g quinhydrone

Electrode Date Code

- The electrode date code indicates the manufacturing date of the electrode.
- Electrodes should be put into service as soon as possible and should not remain in the box for more than two years.
- Over time, the storage solution (found in the "boot" covering the electrode tip) will evaporate or leak, allowing the delicate sensing tip and reference junction to dry.
- To rehydrate a dry electrode, soak it in pH 4 buffer for 24 to 48 hours.
- Electrodes more than 2 years old may still be functional, but will take longer to rehydrate.
- Restoration may not be effective for severely dehydrated electrodes.

	_		
Letter = Month		(K4)	Numeral = Year
N = January	(K4)		5 = 2010
M = February			6 = 2011
L = March			7 = 2012
K = April		_	8 = 2013
J = May		_	9 = 2014
H = June			0 = 2015
G = July			1 = 2016
F = August			2 = 2017
E = September			3 = 2018
D = October			4 = 2019
C = November			5 = 2020
B = December			6 = 2021

Example: K8 = manufactured in April 2013

Electrode Care and Application

pH/ORP electrodes are similar to batteries; they age with time and usage. The following information will help maximize electrode life.

General Tips:

- To ensure uninterrupted operation of critical pH systems, replacement electrodes should be available.
- · Store boxed electrodes flat or upright (electrode tip down) to maximize hydration of the glass surface.
- Keep the glass surface wet at all times.
- Soak the sensor tip in pH 4.0 buffer during system maintenance intervals.
- If the sensor dehydrates, soak the sensor tip in pH 4 buffer for 24 to 48 hours, then visually inspect the electrode for surface cracks, swelling, or discoloration.
- It may not be possible to restore severely dehydrated electrodes to normal operation.
- · High temperatures, strong acids or caustics will increase electrochemical reactions and speed electrode aging.
- Coatings (e.g. grease) on the glass or junction surfaces cause extended response time and inaccurate measurement.
- · Never store the electrode tip in deionized (DI) water. Use pH 4 buffer solution to keep the glass wet when out of the process.
- Never store the electrode at temperatures below 0 °C (32 °F) or allow it to dehydrate.
- · Never scrape or sand the glass electrode surface.
- Treat glass electrode surfaces with care to prevent accidental breakage.

Cleaning

Problem	Suggested Solution
	Use a dilute acid solution (HCl solution of 5% or less). If the electrode has been used in applications with a pH value higher than 7 pH, soak the electrode for 2 to 5 minutes.
Hard Coatings	Use a dilute alkaline solution (NaOH solution at 5% or less) if the electrode has been used in applications with pH values less than 7 pH, soak the electrode for 2 to 5 minutes.
	Alternating immersion in acidic and alkaline solutions may be necessary for thorough cleaning.
Soft Coatings	Spray or vigorously stir the electrode with a mild detergent, such as dishwashing liquid. Chlorine bleach can also be used.
Oily or Organic Coatings	Spray or vigorously stir the electrode with a mild detergent or an appropriate solvent that will not attack the materials of construction. (isopropyl alcohol or similar)
ORP Platinum Coating Gently wipe the electrode surfaces with a paper towel.	
After Cleaning	Always rinse the electrode with water after cleaning.
After Cleaning	Soak the electrode in a pH 4 buffer (with KCl if available) for at least 10 minutes after cleaning.

Ordering Information

2724-2726	and 2734-2730	NH/OPP	Flactrodes
2124-2120	anu 2134-2131	DINURE	Electrodes

**Use with 2750 Sensor Electronics

Mfr. Part No. 3-2724-00 3-2724-01 3-2724-10 3-2724-11 3-2724-HF-10 3-2724-HF-11	Code 159 001 545 159 001 546 159 001 547 159 001 548 159 001 771 159 001 772	Description Electrode, pH, flat, PT1000, ¾ in. NPT Electrode, pH, flat, PT1000, ISO 7/1 R¾ Electrode, pH, flat, 3K Balco, ¾ in. NPT Electrode, pH, flat, 3K Balco, ISO 7/1 R¾ Electrode, pH, HF resistant, flat, 3K Balco, ¾ in. NPT Electrode, pH, HF resistant, flat, 3K Balco, ISO 7/1 R¾			
3-2726-00 3-2726-01 3-2726-10 3-2726-11	159 001 553 159 001 554 159 001 555 159 001 556	Electrode, pH, bulb, PT1000, ¾ in. NPT Electrode, pH, bulb, PT1000, ISO 7/1 R¾ Electrode, pH, bulb, 3K Balco, ¾ in. NPT Electrode, pH, bulb, 3K Balco, ISO 7/1 R¾			
3-2726-HF-00 3-2726-HF-01 3-2726-HF-10 3-2726-HF-11	159 001 549 159 001 550 159 001 551 159 001 552	Electrode, pH, HF resistant, bulb, PT1000, ¾ in. NPT Electrode, pH, HF resistant, bulb, PT1000, ISO 7/1 R¾ Electrode, pH, HF resistant, bulb, 3K Balco, ¾ in. NPT Electrode, pH, HF resistant, bulb, 3K Balco, ISO 7/1 R¾			
3-2726-LC-00 3-2726-LC-01 3-2726-LC-10 3-2726-LC-11	159 001 557 159 001 558 159 001 559 159 001 560	Electrode, pH, bulb, Low Cond, PT1000, ¾ in. NPT Electrode, pH, bulb, Low Cond, PT1000, ISO 7/1 R¾ Electrode, pH, bulb, Low Cond, 3K Balco, ¾ in. NPT Electrode, pH, bulb, Low Cond, 3K Balco, ISO 7/1 R¾			
3-2725-60 3-2725-61	159 001 561 159 001 562	Electrode, ORP, flat, 10 K Ω ID, $\%$ in. NPT Electrode, ORP, flat, 10 K Ω ID, ISO 7/1 R $\%$			
3-2734-00 3-2734-01 3-2734-HF-00 3-2734-HF-01	159 001 774 159 001 775 159 001 776 159 001 777	Electrode, pH, flat, PT1000, ¾ in. NPT ** Electrode, pH, flat, PT1000, ISO 7/1 R¾ ** Electrode, pH, HF resistant, flat, PT1000, ¾ in. NPT ** Electrode, pH, HF resistant, flat, PT1000, ISO 7/1 R¾ **			
3-2736-00 3-2736-01 3-2736-HF-00 3-2736-HF-01	159 001 778 159 001 779 159 001 780 159 001 781	Electrode, pH, bulb, PT1000, ¾ in. NPT ** Electrode, pH, bulb, PT1000, ISO 7/1 R¾ ** Electrode, pH, HF resistant, bulb, PT1000, ¾ in. NPT ** Electrode, pH, HF resistant, bulb, PT1000, ISO 7/1 R¾ **			
3-2735-60 3-2735-61	159 001 782 159 001 783	Electrode, ORP, flat, 10 K Ω ID, $\frac{3}{4}$ in. NPT Electrode, ORP, flat, 10 K Ω ID, ISO 7/1 R $\frac{3}{4}$			
Accessories and Renlacement Parts					

Accessories and Replacement Parts

7 to o o o o ti i o o o o o o o o o o o o				
Mfr. Part No.	Code	Description		
3-2750-1	159 000 744	In-line Sensor Electronics w/Junction Box		
3-2750-2	159 000 745	In-line Sensor Electronics w/Junction Box and EasyCal		
3-2750-3	159 000 746	Submersible Sensor Electronics with 15 ft cable, ¾ in. NPT threads		
3-2750-4	159 000 842	Submersible Sensor Electronics with 15 ft cable, ISO 7/1 R¾ threads		
3-2750-7	159 001 671	pH Electronics, Digital (S³L), 4.6 m (15 ft) cable		
3-2760-1	159 000 939	Submersible Preamplifier with 3/4 in. NPT threads and 4.6 m (15 ft) cable		
3-2760-2	159 000 940	Submersible Preamplifier with 3/4 in. ISO threads and 4.6 m (15 ft) cable		
3-2760-3	159 000 941	Submersible Connector with 4.6 m (15 ft) cable and ¾ in. NPT threads		
3-2760-4	159 000 942	Submersible Connector with 4.6 m (15 ft) cable and ISO 7/1 R¾ in. threads		
3-2760-11	159 001 367	In-line Preamplifier with ¾ in. NPT threads and 4.6 m (15 ft) cable		
3-2760-21	159 001 368	In-line Preamplifier with ¾ in. ISO threads and 4.6 m (15 ft) cable		
3-2760-31	159 001 369	In-line Connector with 4.6 m (15 ft) cable and ¾ in. NPT threads		
3-2760-41	159 001 370	In-line Connector with 4.6 m (15 ft) cable and ISO 7/1 R3/4 threads		
3-2759	159 000 762	pH/ORP System Tester (adapter cable sold separately)		
3-2759.391	159 000 764	2759 DryLoc Adapter Cable (for use with 2750 and 2760)		
3-0700.390	198 864 403	pH Buffer Kit (1 each 4, 7, 10 pH buffer in powder form, makes 50 mL)		
3822-7004	159 001 581	pH 4 buffer solution, pint (16 oz) (473 ml)		
3822-7007	159 001 582	pH 7 buffer solution, pint (16 oz) (473 ml)		
3822-7010	159 001 583	pH 10 buffer solution, pint (16 oz) (473 ml)		
3822-7115	159 001 606	20 gram bottle Quinhydrone for ÓRP calibration		
3-2700.395	159 001 605	Calibration kit: 3 Polypropylene cups, box used as cup stand, 1 pint pH 4.01, 1 pint pH 7.00		
3-8050.390-1	159 001 702	Retaining Nut, Replacement, Valox®, K4530		

+GF+

Georg Fischer Signet LLC, 3401 Aero Jet Avenue, El Monte, CA 91731-2882 U.S.A. • Tel. (626) 571-2770 • Fax (626) 573-2057 For Worldwide Sales and Service, visit our website: www.gfsignet.com • Or call (in the U.S.): (800) 854-4090 For the most up-to-date information, please refer to our website at www.gfsignet.com